

PATENT APPLICATION TRANSMITTAL LETTER

(Large Entity)

Docket No.

772/72321-1

TO THE ASSISTANT COMMISSIONER FOR PATENTS

Transmitted herewith for filing under 35 U.S.C. 111 and 37 C.F.R. 1.53 is the patent application of:

CLINCH

MICROSCOPY

Enclosed are:

- ☐ Certificate of Mailing with Express Mail Mailing Label No.
- ☒ **Three (3)** sheets of drawings.
- ☒ A certified copy of a **Two (2) European** application.
- ☐ Declaration ☐ Signed. ☐ Unsigned.
- ☐ Power of Attorney
- ☐ Information Disclosure Statement
- ☒ Preliminary Amendment
- ☐ Other:

CLAIMS AS FILED

For	#Filed	#Allowed	#Extra	Rate	Fee
Total Claims	9	- 20 =	0	x \$18.00	\$0.00
Indep. Claims	2	- 3 =	0	x \$78.00	\$0.00
Multiple Dependent Claims (check if applicable) <input type="checkbox"/>					\$0.00
BASIC FEE					\$690.00
TOTAL FILING FEE					\$690.00

- ☒ A check in the amount of _____ to cover the filing fee is enclosed.
- ☐ The Commissioner is hereby authorized to charge and credit Deposit Account No. _____ as described below. A duplicate copy of this sheet is enclosed.
- ☐ Charge the amount of _____ as filing fee.
- ☐ Credit any overpayment.
- ☐ Charge any additional filing fees required under 37 C.F.R. 1.16 and 1.17.
- ☐ Charge the issue fee set in 37 C.F.R. 1.18 at the mailing of the Notice of Allowance, pursuant to 37 C.F.R. 1.311(b).

Dated: April 20, 2000

Signature

John P. DeLuca

Registration No. 25,505

cc:

LAWRENCE R. RADANOVIC
RICHARD H. TUSHNET
DONALD N. HUFF
JOHN P. DELUCA

MICHAEL BERGMAN (NY & MA BARS)
SANDRA S. SNAPP

WALTER D. AMES
ROY W. BUTRUM
Of Counsel

LAW OFFICES
WATSON COLE GRINDLE WATSON, P.L.L.C.

10th FLOOR
1400 K STREET, N.W.
WASHINGTON, D.C. 20005-2477

TELEPHONE (202) 628-3600
FACSIMILE (202) 628-3650
PATENT, TRADEMARK, COPYRIGHT
AND RELATED INTELLECTUAL PROPERTY CAUSES

April 20, 2000

ESTABLISHED 1864

ROBERT C. WATSON
COMMISSIONER OF PATENTS
1953-1961

e-mail: RP@WCGW.COM
WCGW@WCGW.COM

Assistant Commissioner for Patents
Washington, D.C. 20231

Re: New U.S. Patent Application
Noah CLINCH
"MICROSCOPY"
Our Reference: 772/7321-2

Dear Sir:

Transmitted herewith for filing is a patent application entitled "MICROSCOPY".
The application is being filed without an oath or declaration pursuant to 37 C.F.R.
1.53(d).

The inventor of the claimed subject matter is:


Noah CLINCH, Kent, Great Britain.

Please address all communications to John P. DeLuca, WATSON COLE
GRINDLE WATSON, P.L.L.C., 1400 K Street, N.W., 10th Floor, Washington, D.C.
20005-2477. Telephone (202) 628-3600.

Respectfully submitted.

WATSON COLE GRINDLE WATSON, P.L.L.C.

By:


John P. DeLuca
Registration No. 25,505

IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

In re Application of:)	PATENT
)	
Noah CLINCH)	Group: To Be Assigned
)	
Serial No.: New Application)	Examiner: To Be Assigned
)	
Filed: On Even Date)	
)	
MICROSCOPPY)	

PRELIMINARY AMENDMENT

Assistant Commissioner for Patents
Washington, D.C. 20231

Washington, D.C.
April 20, 2000

Sir:

Prior to initial examination on the merits, please amend the above-identified application as follows:

IN THE CLAIMS:

Claim 2, line 1, change "A" to --The--;

Claim 3, line 1, change "A" to --The--; and delete "or claim 2";

Claim 4, line 1, change "A" to --The--; and delete "2 or 3";

Claim 6, line 1, change "An" to --The--;

Claim 7, line 1, change "An" to --The--; and delete "or claim 6";

Claim 8, line 1, change "An" to --The--; and delete "6 or 7";

Claim 9, line 1, change "An" to --The--.


In the event any multiple dependencies remain in the claims, it is respectfully requested that said multiple dependencies be deleted and reference be made to the immediately preceding claim.

REMARKS

The application has been amended in order to delete multiple dependencies from the claims.

Examination on the merits is earnestly solicited.

Respectfully submitted,



John P. DeLuca
Registration No. 25,505

WATSON COLE GRINDLE WATSON, P.L.L.C.
1400 K Street, N.W., 10th Floor
Washington, D.C. 20005-2477
Phone: (202) 628-3600 Fax: (202) 628-3650
JPD:er

MICROSCOPY

The present invention relates to telemicroscopy and microscopy training.

5 Telemedicine, by which a range of data, such as x-rays or ECG traces, relating to a patient is transmitted from one location to another for diagnosis or a second opinion, is the focus of much attention because of its potential to improve the quality of healthcare while reducing costs.
10 There have been many attempts at developing telemedical applications involving the use of microscopes, such as telepathology and telecytology. All involve the capture of digital or analogue images from a microscope and transmission of these images to a remote site for the
15 purpose of a second opinion or remote diagnosis. However, as will be described, none of the existing systems has been entirely satisfactory.

20 A fundamental problem in the field of telemicroscopy is that the field of view of the microscope is tiny in relation to the size of the specimen on the microscope slide. By way of example, a typical cytology 'smear' will occupy an area of at least 20mm by 50mm, that is 1000mm². The field of view of a typical 20x magnification objective lens is only about 0.4mm by 0.4mm, or 0.16mm². The entire
25 image can therefore be considered to be formed by over 6000 distinct fields. A remote consultant will not want to make a diagnosis on the basis of just a few images selected by another worker, he will want to have access to the whole of the slide and to be able to change or have changed the
30 magnification as and where he wishes.

35 The simplest solution to this problem is a procedure known as static tele-microscopy. In its very basic form, all that is required is a camera coupled to the microscope, some basic software, a network connection such as via the Internet to a remote display, and means for voice communication between the two locations. The microscope is operated by a local worker who will typically, based on

their own knowledge, select an initial area for review by the remote consultant. An image of that area will be acquired and transmitted to the remote consultant's monitor. Based upon what he can see, he relays instructions over the telephone to the local worker - left, right, up, down, increase magnification, etc. Further images are acquired and relayed to the consultant until he is satisfied that he has sufficient information upon which to base his diagnosis. Such static telepathology systems have the virtue of simplicity and low cost. However, trials have repeatedly confirmed that it is unsatisfactory in practice to rely upon a few fixed images and few consultants will be prepared to offer an opinion or make a diagnosis on this basis.

An improved system is known as dynamic telemicroscopy. Essentially, once the slide has been prepared locally, the microscope itself is operated remotely by the remote consultant. Examples are shown in US-A-5 216 596 and US-A-5 297 034. An example has also been placed on public access via the Internet by the Department of Pathology at the Charite Hospital in Berlin (<http://amba.charite.de/telemic/index.html>). However, such on-line systems are expensive both in terms of buying the equipment and in terms of the consultant's time. These systems also need high bandwidth telecommunications, typically at least 384 kbits/sec for even only moderately satisfactory use. Whilst the consultant has full control over the microscope, there are delays whilst instructions are relayed to the microscope, the microscope is adjusted in accordance with those instructions, and the new image is obtained and relayed to the consultant. Such systems cannot strictly be considered to operate in real-time. For a comparison, whilst a consultant operating a local microscope could perhaps examine a sample and provide a diagnosis in a straightforward case in around a minute or perhaps 3 or 4 minutes for a more involved diagnosis, whereas even with dynamic telemicroscopy and experienced

operators each examination can take in the order of ten minutes or so.

There is therefore a need for an improved method of telemicroscopy.

5 The invention also relates to the area of microscopy training, and particularly to the area of teaching of diagnostic methods employing microscopy.

At present training in diagnostic microscopy performed either by circulating prepared sections on glass slides
10 formed by the circulation of electric microscopy images of a data storage medium such as CD ROM. The former of these two approaches is time consuming and inconvenient, particularly because samples get misplaced or damaged in transit. Both methods have the further disadvantage that
15 there is both specific monitoring of whether or not a student performs a diagnosis simply by chance or by incorrect methods, meaning that both are limited teaching tools.

In the context of telemicroscopy and indeed any form
20 of microscopy where images are displayed on a monitor rather than viewed directly by the eye, it is perhaps misleading to talk in terms of magnification. If an image is obtained and displayed full screen on a 17 inch computer monitor, the magnification will be greater than if the same
25 image is displayed full screen on a 15 inch monitor. The resolution will, however, be the same. Accordingly, the term resolution is a better descriptor of the amount of information given in a particular image and relates, in the context of a digital camera, to the number of pixels of the
30 CCD device per unit area of field of view.

According to the present invention, there is provided, in one aspect, a method of telemicroscopy comprising the steps of: preparing a specimen on a microscopy slide; placing the slide upon the stage of a microscope equipped
35 with digital imaging apparatus and motorised stage; imaging the specimen to obtain a composite high resolution image of the whole specimen; digitally obtaining a relatively low

resolution copy of that image; and storing the images in a datastore; wherein the method further comprises the steps of allowing access to the datastore from a terminal; transferring the low resolution image to the terminal and displaying the image upon a monitor; selecting by means of the remote terminal, as desired, an area of the low resolution image and transferring corresponding high resolution image data for that area from the datastore to the terminal.

10 The terminal may be a remote terminal.

The method may comprise the step of recording the areas of the low resolution image that are selected, for review of performance of a person performing the method.

15 In a second aspect, the present invention provides a telemicroscopy apparatus comprising a microscope provided with a digital imaging apparatus and a motorised stage which can be controlled to obtain a digital image or plurality of such images, at a desired high resolution, of an entire specimen placed upon the stage; image processing means to obtain a low resolution copy of the image of the specimen; storage means to store the images obtained; and means for transferring, in use, image data to a terminal in response to requests therefrom.

20 Preferably, the digital imaging apparatus is a digital camera, or else an analogue video camera provided with appropriate digitiser hardware. The apparatus may comprise means for moving the objective lens of the microscope in order to provide automatic focussing.

25 In a preferred embodiment, a continuous sequence of successive images of the specimen is obtained by advancing the field of view of the objective lens of the microscope stepwise across the specimen and acquiring an image of each field of view. The objective lens is selected to ensure sufficient resolution in the images of the specimen and sufficient images are captured and stored to cover the whole area of the specimen on the microscope stage.

The apparatus may comprises means for recording what image data is requested for review of the performance of a user. The recording means maybe a data storage disk, such as a floppy disk.

5 With a knowledge of the pixel size and number in the imaging apparatus used and the calibrated magnification of the objective of the microscope, the computer moves the stage such that adjacent images are effectively continuous in the two dimensional specimen plane, and can be thought
10 of as 'tiles' in a very large composite 'montage' virtual image.

The above and other aspects of the present invention will now be described in further detail, by way of example only, with reference to the accompanying figures, in which:

15 Figure 1 illustrates schematically an embodiment of the apparatus in accordance with the present invention;

Figure 2 is complete navigational map of a sample on a microscope slide which has been imaged in accordance with an embodiment of the method of the present invention; and

20 Figure 3 illustrates in further detail one aspect of the embodiment of Figure 1.

Referring to the Figures, a biopsy sample for analysis is taken and mounted upon a microscope slide 10 in a conventional manner. The specimen slide 10 is placed upon
25 a motor driven stage 11 of a microscope 12 fitted with a camera 13, typically a digital, high resolution CCD camera of diagnostic quality - at least 1024 x 1024 pixels, 24 bit colour. The stage is adjustable in three dimensions with respect to the focal axis of the objective. This is
30 typically achieved with a computer 16 controlled motorised movable stage 11, but could equally well, if unconventionally, be achieved with a static stage and a movable objective.

The objective lens 14 is selected according to the
35 maximum desired resolution for the task in hand - typically 10X, 20X or 40X. The complete specimen is imaged by capturing an image of a first field (or area of the

09553013-040000

specimen) 20, advancing the stage to an adjacent field 21, capturing an image of that field, indexing to the next field 22 and so on (referred to as scanning). The individual field images 20, 21, 22 etc are stored on disk as part of a single large file or may be digitally compressed and stored electronically representing a high resolution virtual image of the original slide specimen. At the same time, a decimated copy of the very large image is created to represent a low resolution navigation map 30. Typically, the number of pixels in the low resolution map 30 will be the same as that in each of the original images 20, 21, for example 1024 x 1024. The total time for acquisition of the collection of high resolution images will typically be around 5-20 minutes, depending, of course, upon the specimen area to be scanned and the field of view of the objective lens.

When scanning with the high power objective, a problem is often encountered in that it is difficult to drive the motorised stage, such that it is normal to the optical axis of the microscope. Indeed, microscope slides are not perfectly flat. Because of this, the need arises to refocus the microscope periodically when scanning a specimen. Refocussing adds significantly to overall scan time. This can be overcome with the present invention by means of a piezo-electric driver, or other objective lens moving device, rather than requiring the movement of the motorised stage relative to a fixed objective lens.

This occurs before the consultant becomes involved and so maintains a high efficiency in terms of consultant time.

In practice, based on a knowledge of the pixel size and number in the camera and the calibrated magnification of the objective of the microscope, the distance by which the stage must move between each image acquisition is calculated. The stage is moved to the co-ordinates of the selected starting point and the first image is acquired. The image is compressed and stored to disk and a low-resolution tile is made from that image. With a

00553043.042000

knowledge of where the tile image originated, the tile is "pasted" onto a navigation map matrix and stored. The stage is then advanced to the next co-ordinates and the next image is acquired.

5 By making use of multi-thread software design, it is possible to optimise scan time by arranging for image compression and storage to run in parallel with stage movement and image acquisition.

10 The microscope stage 11 and the CCD camera 13 are controlled by appropriate hardware and software of the server 15, in a generally conventional manner.

As is evident from the image shown in Figure 2, unevenness in specimen illumination may lead to a certain degree of shading around the periphery of each field image. 15 If desired, the high resolution image can be digitally processed to remove this shading. However, it is envisaged that consultants will generally prefer to see a "raw" image for fear of the loss of important detail if the image is excessively post-processed.

20 The navigation map 30 and collection of high resolution images are stored locally in computer memory in a computer or server 15. For a typical 20 x 50 mm specimen as described in the introduction, such a collection of high resolution images could be expected, with 50-100-fold 25 digital compression, to occupy up to around 1Gb of memory. Typically, a compressed navigation map might be expected to occupy around 50Kb of memory.

At this stage, access to the microscope is no longer required and it can be put to use on the next slide. 30 Communication may now be made between the local server 15 and the consultant at a remote computer 16, upon which is mounted the appropriate client software. Communication may be via a dedicated link, for example to a centralised expert diagnostic centre, or by any other suitable means, 35 such as over the Internet even to a consultant's portable computer. The system is not limited to one:one connections.

The server can be configured to support simultaneous access by multiple clients.

At his client computer 16, the consultant receives the low resolution 'navigation map' 30 of the entire specimen image from which he can access the high resolution images. As the compressed navigation map is comparatively small, there is only a minimal delay whilst the data is transferred. In its simplest form, an original high resolution image itself is retrieved simply by clicking or otherwise selecting the appropriate area in the navigation map 30. In another embodiment, the consultant is able to select any specific area of interest by "rubber banding" a rectangular region either on the client's navigation map display, or else on the currently displayed field of view. The server then extracts the appropriate high resolution image from a very large compressed file, then compresses this field-of-interest view and sends it to the client computer 16.

Typically, the consultant will have two computer monitors, the first monitor 35 to continually display the navigation map 30 and the second monitor 36 to allow the consultant to display a high resolution image 40 of an area 41 selected by the consultant by "rubberbanding" a desired area from the map 30 using, for example, a mouse connected to his terminal. The server 15 will immediately access the image store and construct a compressed image corresponding to the selected area for transmission to the client computer. In the limit of magnification, the enlarged image 40 on the second monitor 36 will typically correspond to the magnification used in the scanning procedure, but it could typically be digitally enlarged up to around twice the scanned magnification without loss of apparent image quality.

In a further preferred embodiment the remote consultant will be able to reconstruct the navigation map. If for example, it is clear at first sight that 50% of the navigation map 30 shows nothing at all or is not relevant

09553043: 042000

to the diagnosis, it may be distracting for the consultant to have it constantly displayed on the first screen 35. Accordingly, the consultant can 'rubberband' the desired area and the server will construct a new navigation map and transmit it to the client computer. Thus the new navigation map may be at the same resolution as the original map or at an increased resolution as desired.

An advantage of the present system is that the complex and storage intensive data processing is carried out by the server 15 locally to the microscope, such that only that image data called upon by the consultant needs to be transmitted to the consultant's computer 16. That data is comparatively small and can thus be transmitted quickly. The client computer 16 is not required to carry out any complex data processing other than decompression and display of the images retrieved from the server. In addition, the server can be configured to allow multiple concurrent accessing of the data, for the purposes, for example, of multiple diagnosis or teaching.

In the preferred embodiment illustrated, the second monitor 36 also displays small thumbnail images 45 of areas previously examined in detail as an enlarged image 41. These thumbnail images 45 are temporarily stored locally to facilitate rapid retrieval should the consultant so require. Ultimately, the original image data corresponding to the thumbnail images, and including the navigation map image 30, can be stored centrally constituting a part of the patient's medical records and also serving as an audit trail recording those areas of the slide which were actually examined by the consultant. The remaining high resolution images on the server can be discarded or backed up as desired. This illustrates a yet further advantage of the present invention. It is inherently well adapted for efficient data warehousing and provides a useful compromise between storing the whole data and storing no data. Neither of the existing dynamic or static telemicroscopy techniques

can provide such a feature without considerable additional modification.

Use of the present invention allows the remote consultant access to any area of the slide at will, and
5 allows him to control magnification at will. In many applications, it is as fast as direct examination of the local slide.

Having described the use of two screens, it will be immediately apparent that the same result can be achieved
10 using separate virtual screens or windows within a GUI operating system upon the same monitor screen.

The apparatus and method of the present invention are particularly well suited to the majority of occasions where an immediate diagnosis is not required and its primary
15 advantage is in the speeding up of non-urgent cases. It avoids the need for microscope samples to be transferred between hospitals, being advantageous both in terms of reducing the delays due to samples being in transit and the risks associated with transferring possibly dangerous
20 samples. However, the invention is also potentially suitable for those cases where an immediate diagnosis is required, for example when a frozen section sample has been taken from a patient during an exploratory operation. This feature will be particularly advantageous in highly
25 specialised areas of medicine in which there may be only a few suitably experienced clinicians who may well be in other parts of the world when a diagnosis is required.

In summary, the present invention overcomes the stated limitations of static telemicroscopy without the high cost
30 entailed in dynamic telemicroscopy. Cost saving is primarily through reduction of consultant time. This is essential to realise the potential benefits to quality of diagnosis in routine telepathology etc. Furthermore, the scanning process can easily be adapted to unattended hatch
35 processing, in which, not just one slide but a collection of slides is scanned sequentially.

0055043:040000

The simplicity of providing multiple access to the server makes the invention ideal for teaching purposes, as well as for professional quality assurance assessment.

The concepts described above can be applied as a teaching apparatus and for professional quality assurance by providing the apparatus with a return path in which the apparatus returns information about the fields of view selected by the operator. The apparatus may also provide means for enabling annotation to be inserted by a user to provide total feedback of the user's approach to a monitoring teacher.

With such an arrangement it is not necessary to return actual images, but simply to return the bounds information on the boundaries of the field within the frame of reference of the large-scale virtual image. This is because the teacher has access to an exact copy and reconstruction can be performed at the teacher's server. In this way, an entire diagnostic session can be returned in a file which can be easily transmitted by E-mail or on a floppy disk, for example.

Whilst, as with the above example, the image provider (teacher) and the image reviewer (the student) can be at either end of a local area network or other telecommunications, other possibilities are available. For 25 example an appropriate data storage device, such as a CD-ROM could incorporate all of the image data and when loaded into an appropriately configured PC can emulate a remotely accessed system.

CLAIMS

1. A method of telemicroscopy comprising the steps of:
5 preparing a specimen on a microscopy slide; placing the
slide upon the stage of a microscope equipped with digital
imaging apparatus and motorised stage; imaging the specimen
to obtain a composite high resolution image of the whole
specimen; digitally obtaining a relatively low resolution
10 copy of that image; and storing the images in a datastore;
wherein the method further comprises the steps of allowing
access to the datastore from a terminal; transferring the
low resolution image to the terminal and displaying the
image upon a monitor; selecting by means of the remote
terminal, as desired, an area of the low resolution image
15 and transferring corresponding high resolution image data
for that area from the datastore to the terminal.
2. A method according to claim 1, wherein the terminal is
a remote terminal.
- 20 3. A method according to claim 1 or claim 2, further
comprising the step of recording the areas of the low
resolution image that are selected, for review of
performance of a person performing the method.
- 25 4. A method according to claim 1, 2 or 3, wherein a
continuous sequence of successive images of the specimen is
obtained by advancing the field of view of the objective
lens of the microscope stepwise across the specimen and
30 acquiring an image of each field of view.
5. A telemicroscopy apparatus comprising a microscope
provided with a digital imaging apparatus and a motorised
stage which can be controlled to obtain a digital image or
35 plurality of such images, at a desired high resolution, of
an entire specimen placed upon the stage; image processing
means to obtain a low resolution copy of the image of the

00553043 042000

specimen; storage means to store the images obtained; and means for transferring, in use, image data to a terminal in response to requests therefrom.

5 6. An apparatus according to claim 5, wherein the digital imaging apparatus is a digital camera.

7. An apparatus according to claim 5 or claim 6,
10 comprising means for moving the objective lens of the microscope in order to provide automatic focussing.

8. An apparatus according to claim 5, 6 or 7 comprising means for recording what image data is requested for review of the performance of a user.

15 9. An apparatus according to claim 8, wherein the recording means is a data storage disk, such as a floppy disk.

000270 34055550

ABSTRACT

A method of telemicroscopy comprises the step of preparing a specimen on a microscopy slide. The slide is placed upon the stage of a microscope equipped with digital imaging apparatus and motorised stage and the specimen imaged to obtain a composite high resolution image of the whole specimen. A relatively low resolution copy of that image is obtained and stored in a datastore. The method further comprises the steps of allowing access to the datastore from a terminal transferring the low resolution image to the terminal and displaying the image upon a monitor selecting by means of the remote terminal, as desired, an area of the low resolution image and transferring corresponding high resolution image data for that area from the datastore to the terminal.

000240.240550

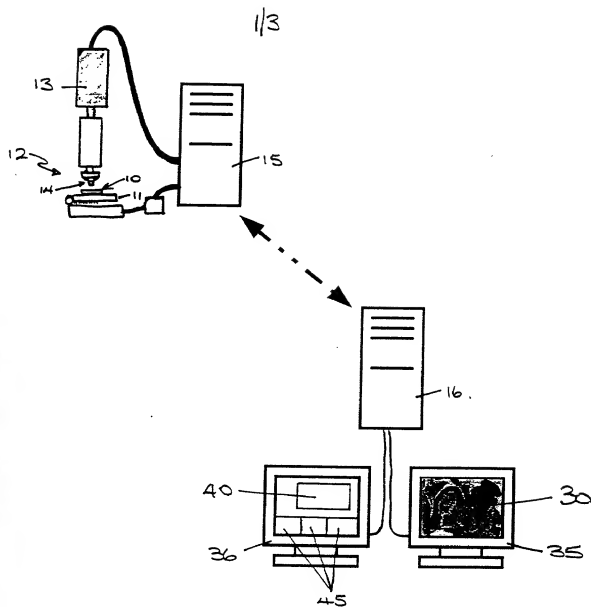


FIGURE 1.

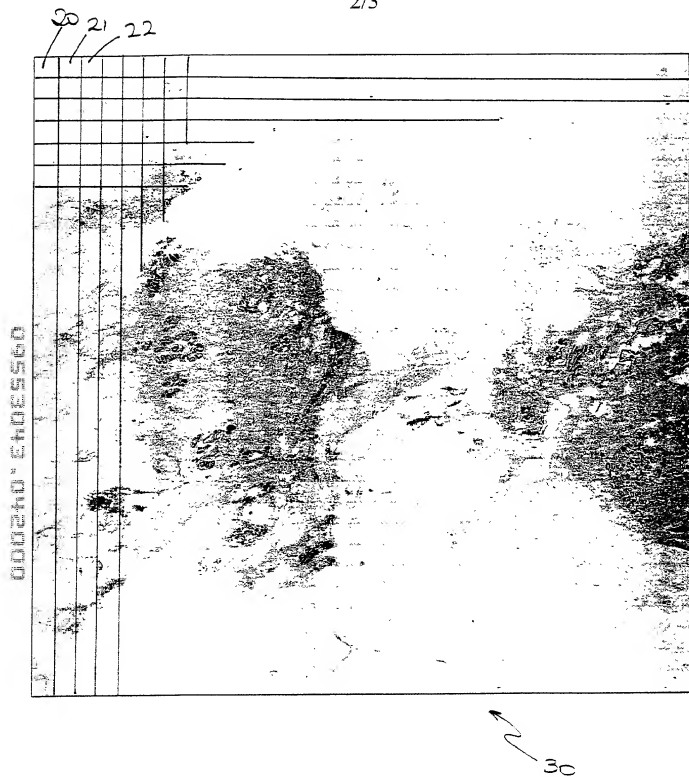


Figure 2

000240-8405560

Figure 3.

